





1/5

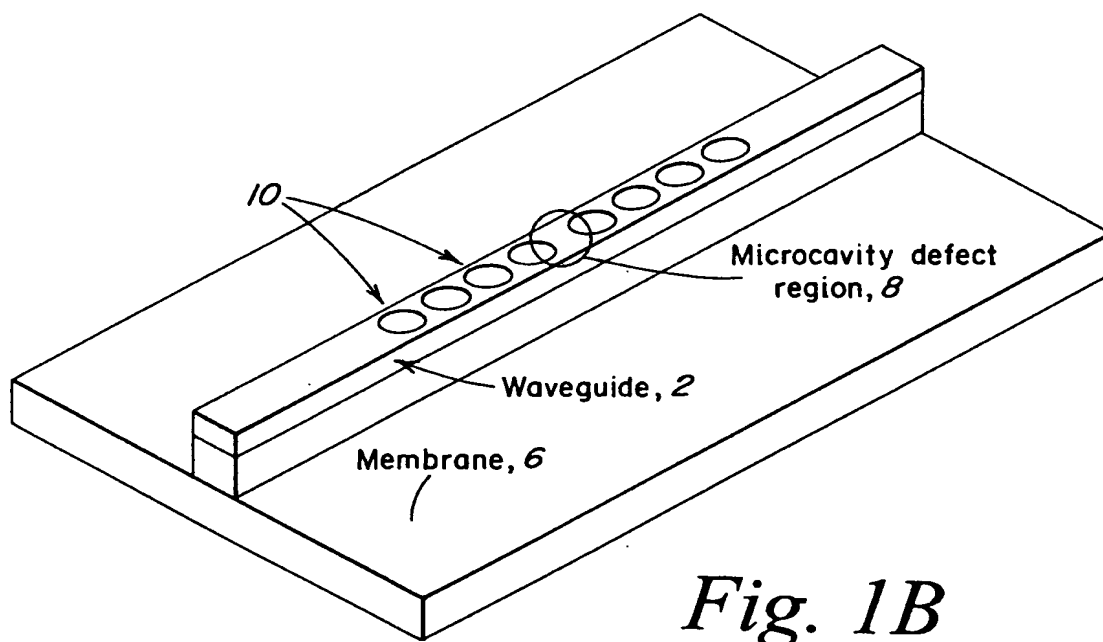

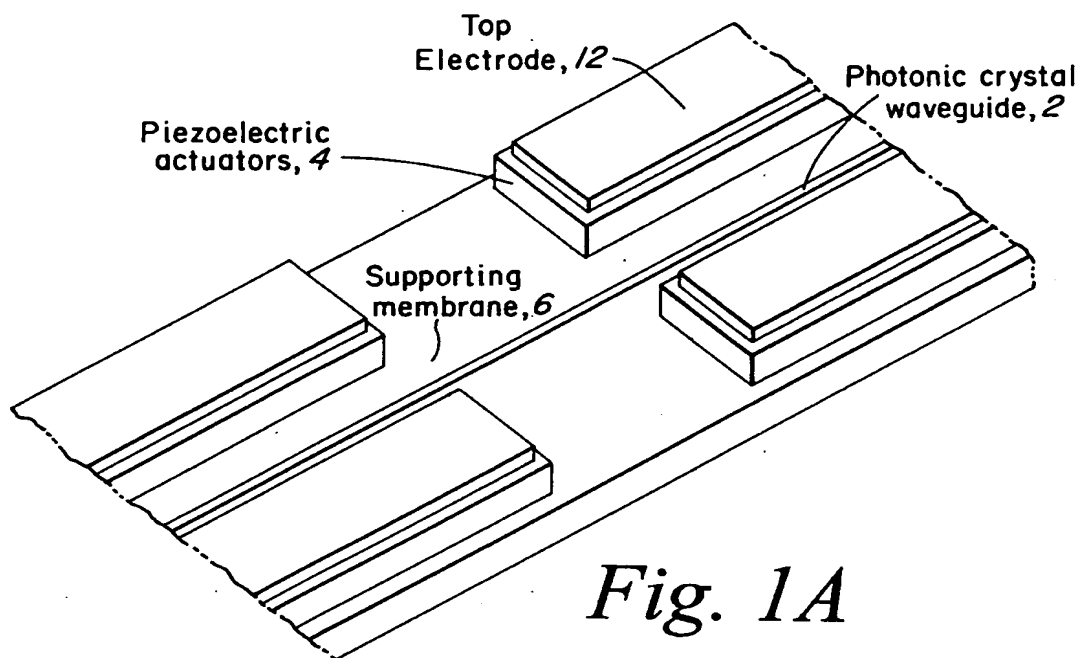

2/5

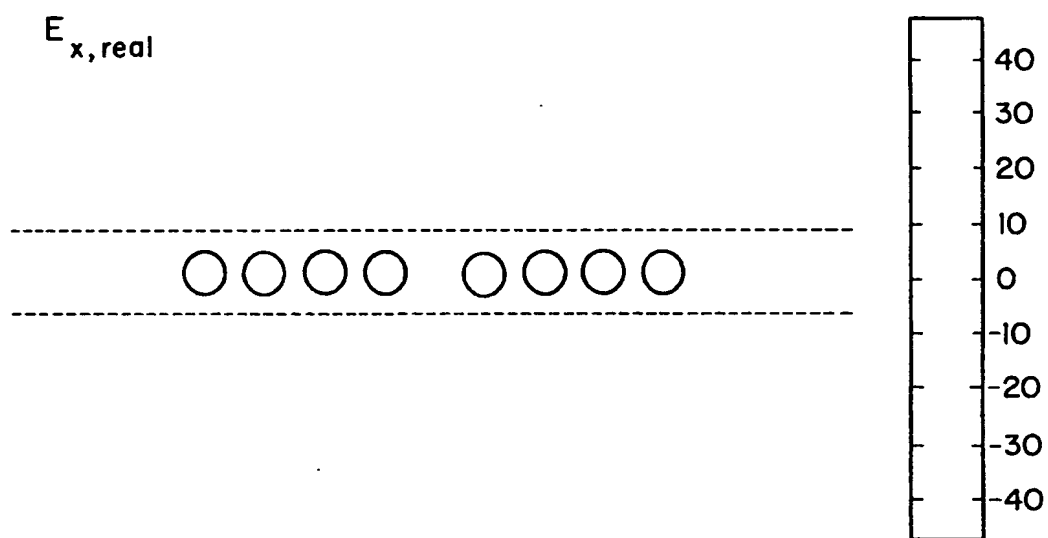


Fig. 2



3/5

STRAIN II
RST CALC
TIME 1.000

0.002100
0.001500
0.000900
0.000300
-0.000300
-0.000900
-0.001500

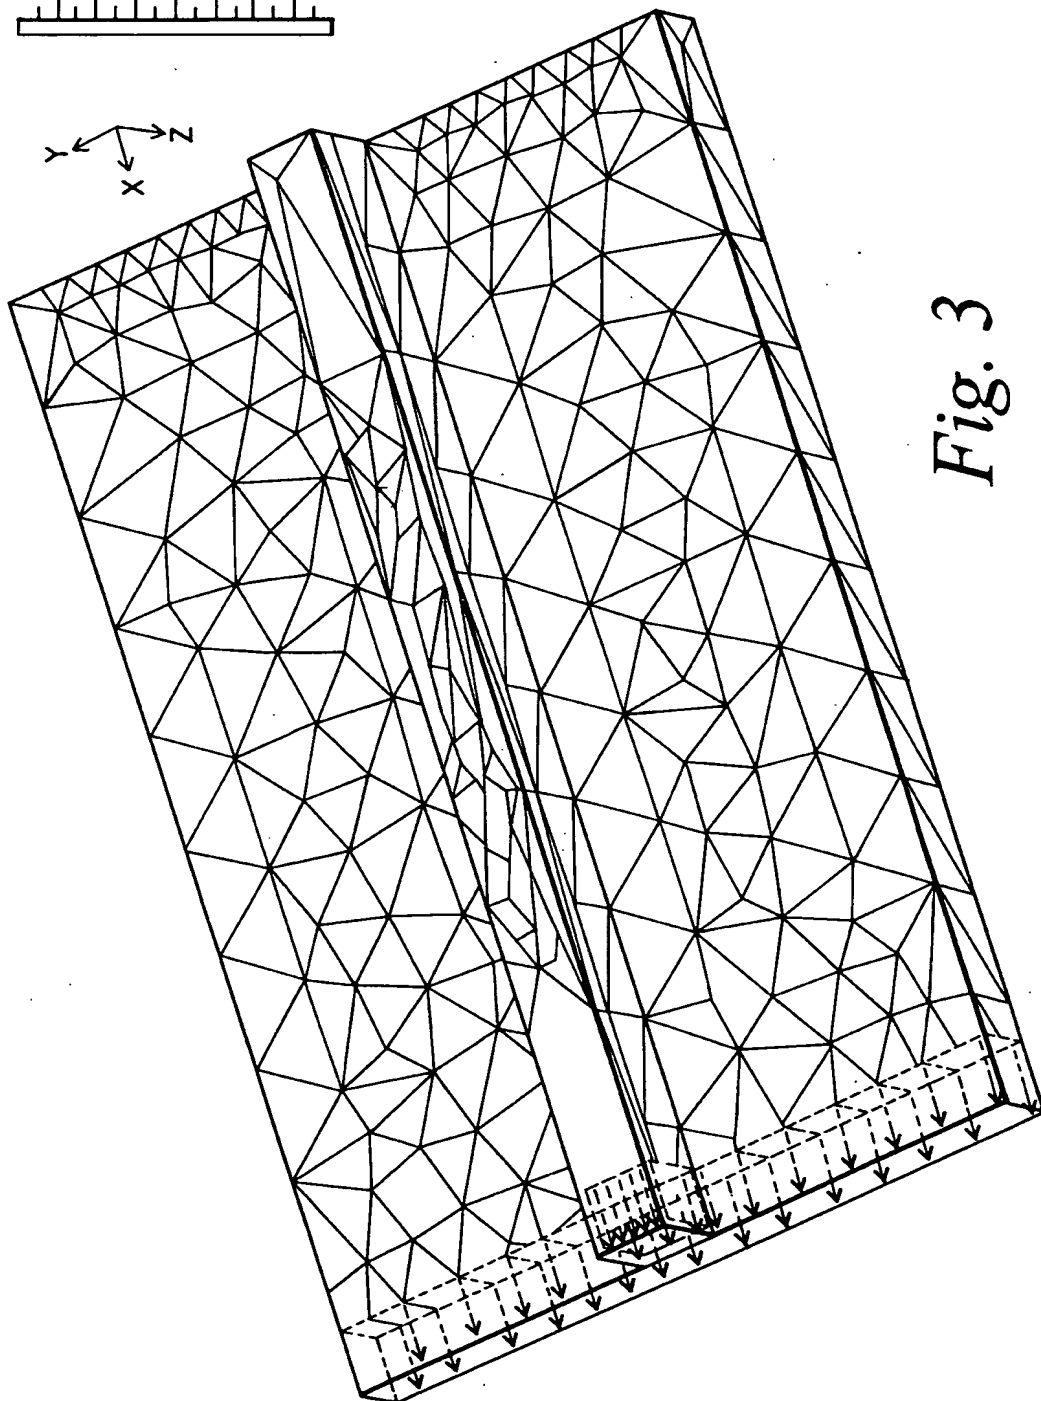


Fig. 3

4/5

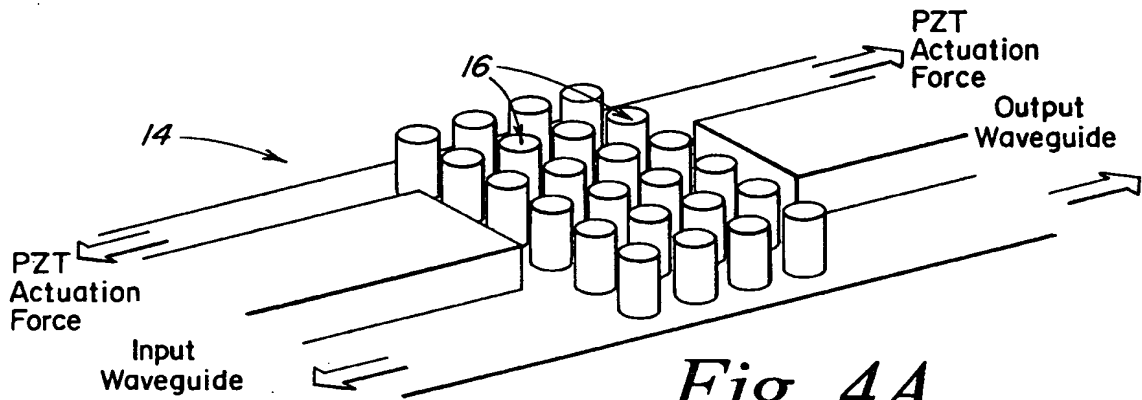


Fig. 4A

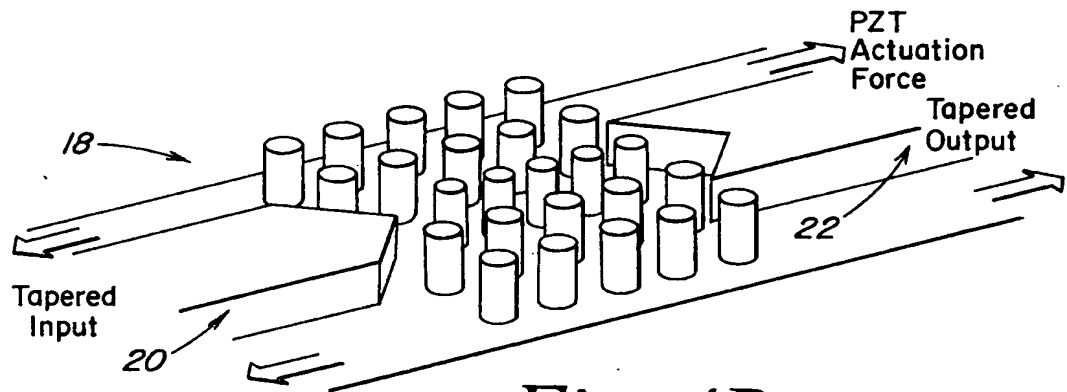


Fig. 4B

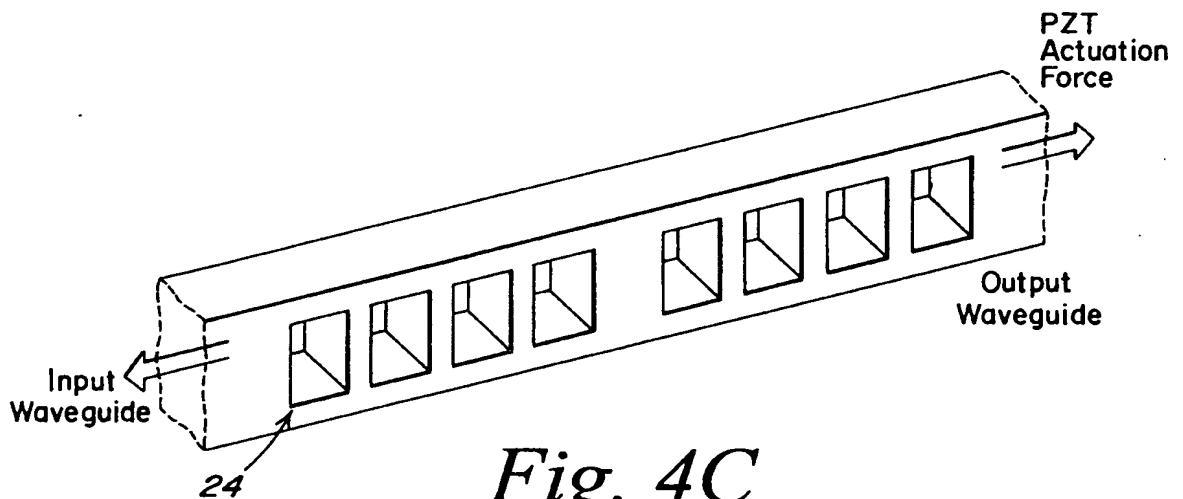


Fig. 4C



5/5

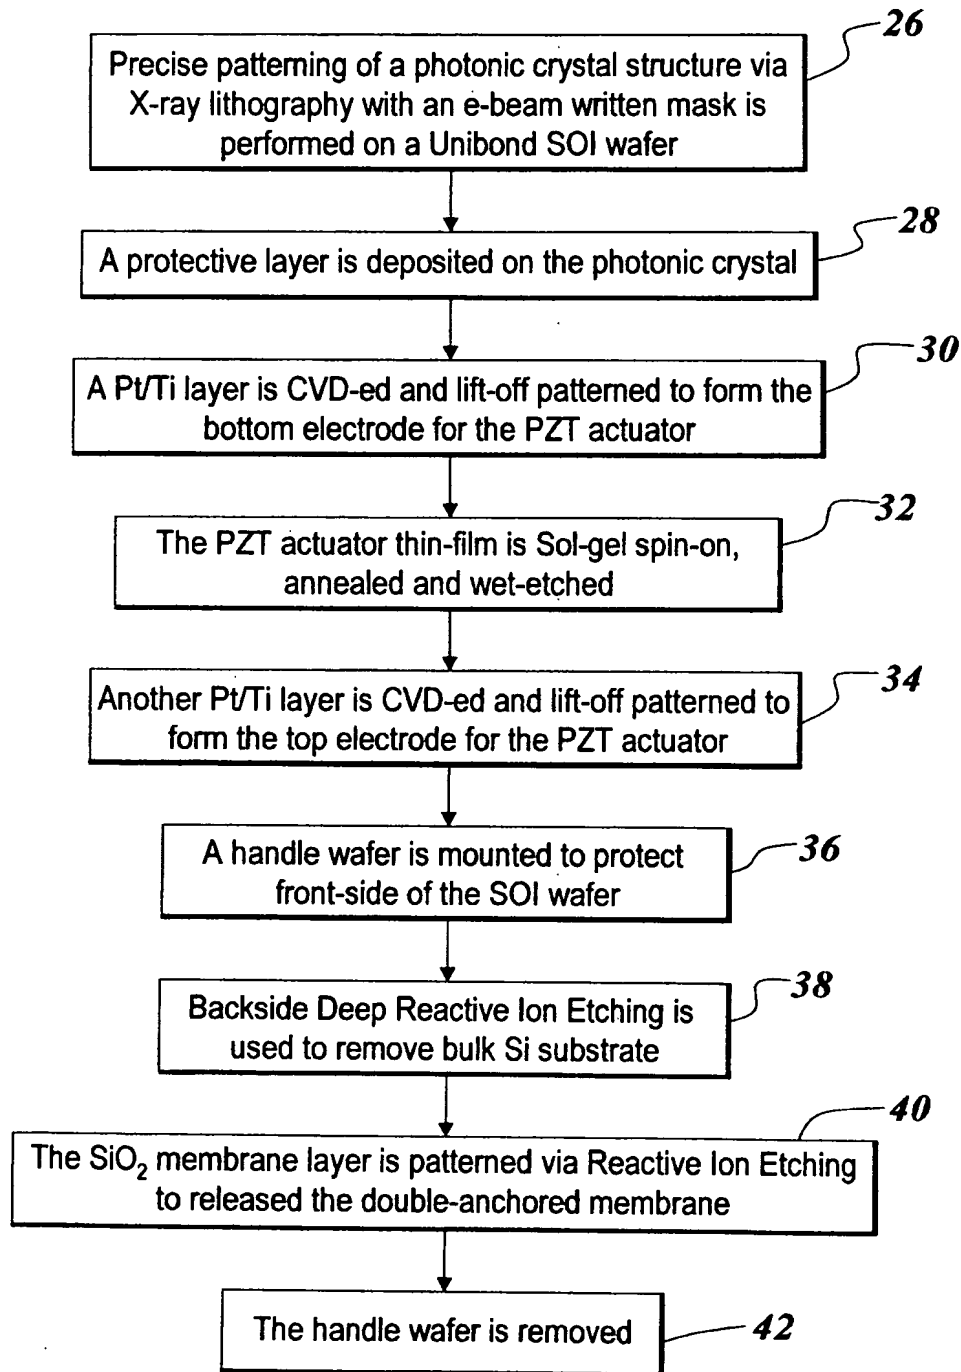


Fig. 5